RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

Dräger medical
A Dräger and Siemens Company

# Field Service Procedure

Part Number: SP00286
Rev: -
Date: 15 September 2003
© 2003 Draeger Medical, Inc.

# Double Vapor Parking Installation

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

# ASSEMBLY AND INSTALLATION OF DOUBLE VAPOR PARKING ACCESSORY

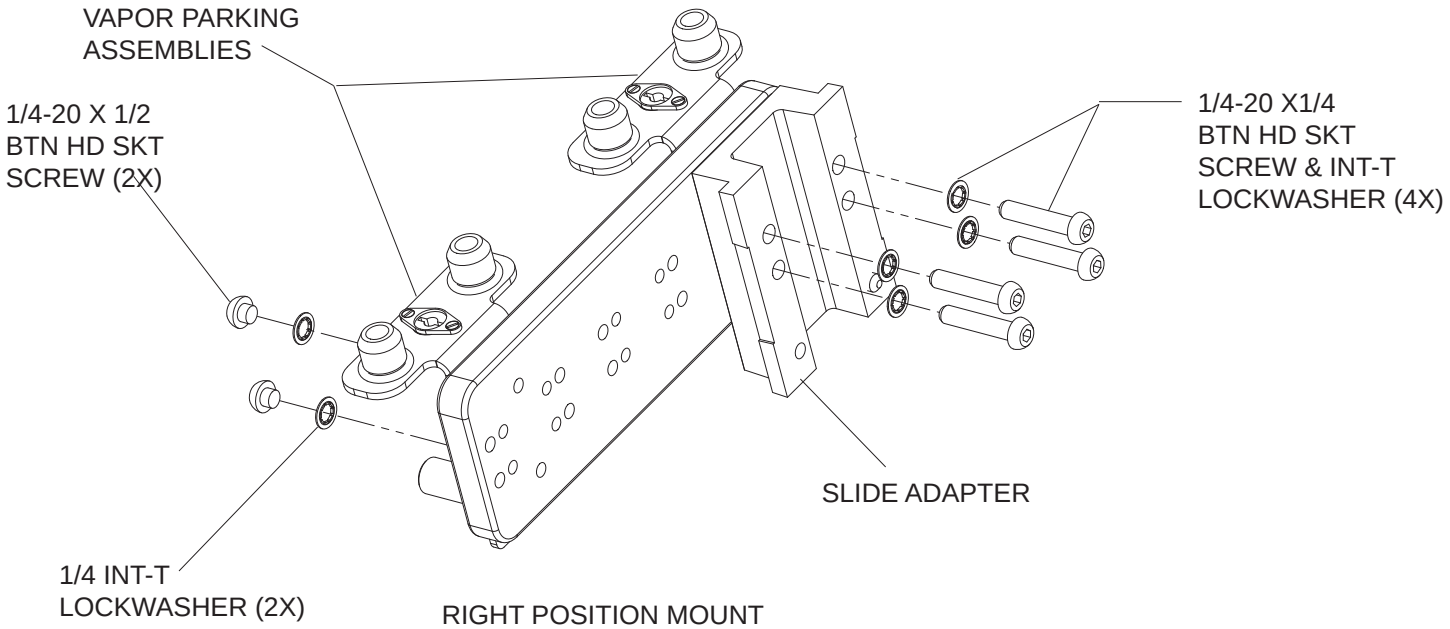


RIGHT POSITION MOUNT
RIGHT SIDE
FABIUS GS, NM6000 & FABIUS TIRO

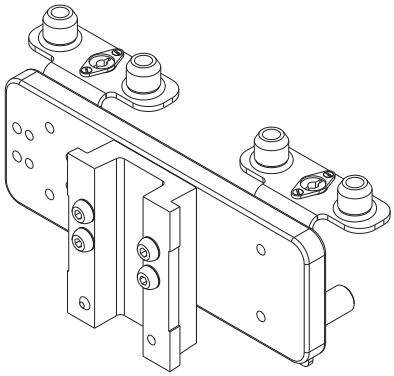

CENTER POSITION MOUNT
FABIUS GS & NM6000

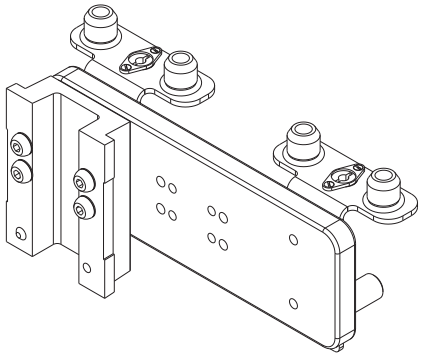

LEFT POSITION MOUNT
RIGHT SIDE
FABIUS GS, NM6000 & FABIUS TIRO

1. Select a permitted double vapor parking arrangement (left, center or right position).
2. Attach the slide adapter to the mounting plate with four 1/4-20 x 1-1/4 in. btn hd skt screws and 1/4 int-t lock washers as shown in the illustration.
3. Attach each vapor parking assembly to the mounting plate as shown in the illustration with two 1/4-20 x 1/2 in. btn hd skt screws and 1/4 int-lock washers.

Installation:Continued:

Note: Machine must be equipped with a GCX rail.

4. Install the double vapor parking accessory in the GCX rail. Position the stop piece in the GCX rail at the selected position and tighten the setscrews.

WARNING: Do not install the double vapor parking accessory on the left side GCX rail on a Narkomed 6000 Series Machine.

TYPICAL NM6000 INSTALLATIONS:

LEFT POSITION MOUNT

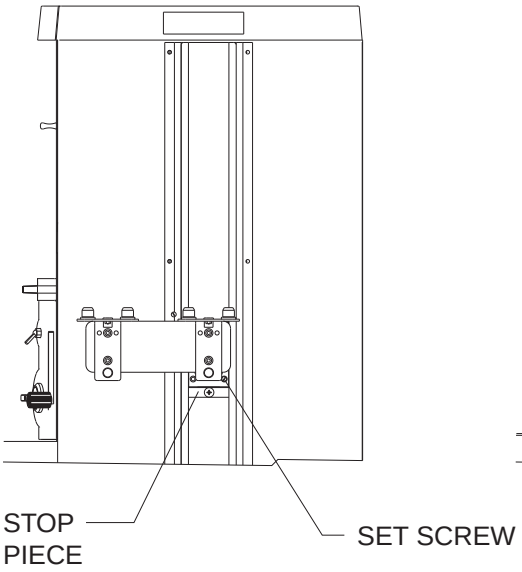


CENTER POSITION MOUNT

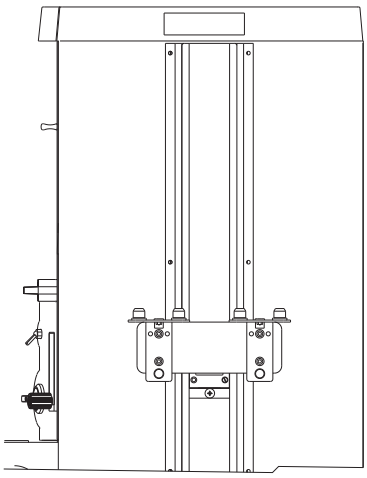

RIGHT POSITION MOUNT

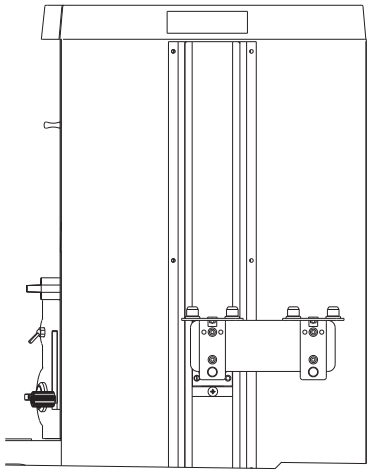

TYPICAL FABIUS TIRO INSTALLATION:

RIGHT POSTION MOUNT
(FOR USE WITH LEFT MOUNTED BREATHING SYSTEM ONLY)

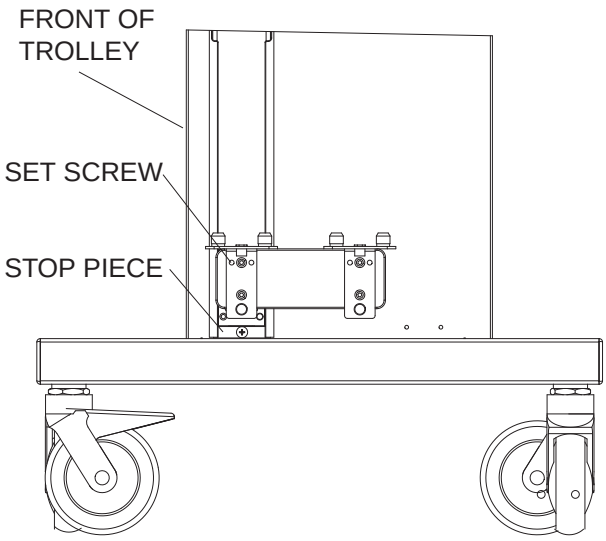


LEFT POSTION MOUNT
(FOR USE WITH RIGHT MOUNTED BREATHING SYSTEM ONLY)

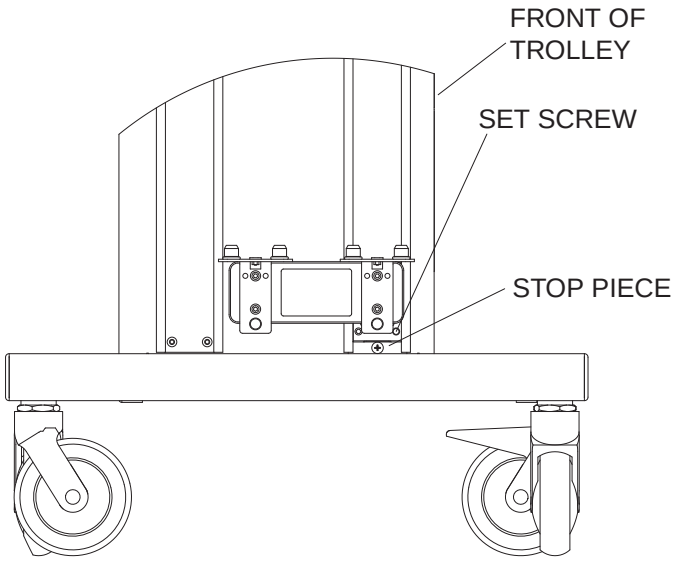

# VAPOR PARKING ASM

TYPICAL FABIUS GS INSTALLATIONS:

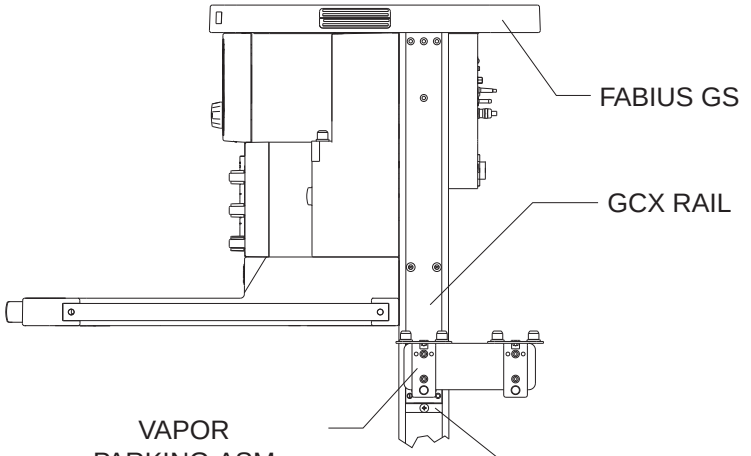


VAPOR
PARKING ASM
RIGHT POSITION MOUNT
(POSITION ONLY
BELOW HANDLE)

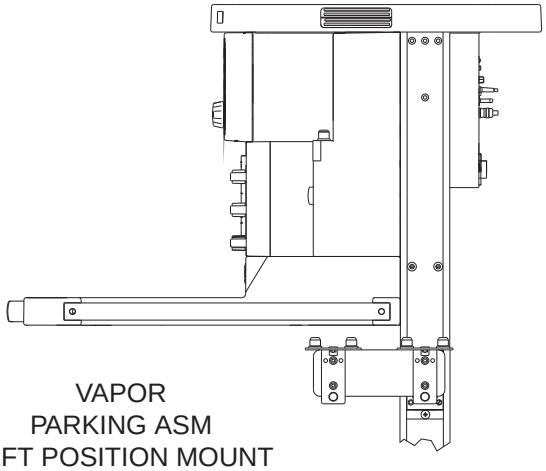

VAPOR
PARKING ASM
LEFT POSITION MOUNT
(BELOW HANDLE ONLY)

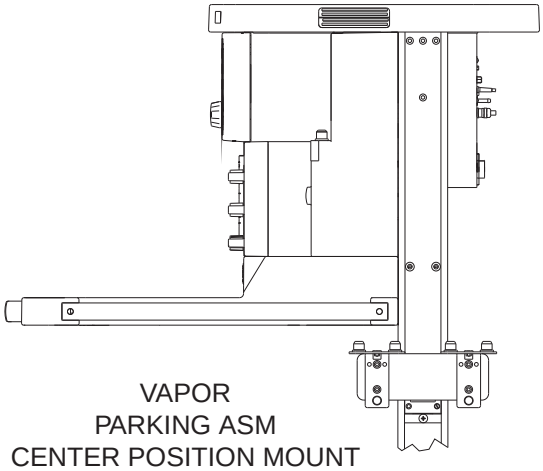

VAPOR
PARKING ASM
CENTER POSITION MOUNT
(BELOW HANDLE ONLY)

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

Dräger medical

A Dräger and Siemens Company

DrägerService is a division of
Draeger Medical, Inc.
3122 Commerce Drive
Telford, PA 18969
Tel: (215) 721-5402
(800) 543-5047
Fax:(215) 721-5784
Web: www.draegermedical.com
Printed in the U.S.A.